



KERN & Sohn GmbH

Ziegelei 1
D-72336 Balingen
E-Mail: info@kern-sohn.com

Phone: +49-[0]7433-9933-0
Fax: +49-[0]7433-9933-149
Internet: www.kern-sohn.com



Operating manual Compact balance

KERN FOB-N

Version 1.1
05/2016
GB



FOB-NS



FOB-NL

FOB-N-BA-e-1611



KERN FOB-N

Version 1.1 05/2016

Operating manual Compact balance

Contents

| | | |
|----------|---|-----------|
| 1 | Technical data | 4 |
| 2 | Basic Information (General) | 6 |
| 2.1 | Proper use | 6 |
| 2.2 | Improper Use | 6 |
| 2.3 | Warranty | 6 |
| 2.4 | Monitoring of Test Resources..... | 7 |
| 3 | Basic Safety Precautions | 7 |
| 3.1 | Pay attention to the instructions in the Operation Manual..... | 7 |
| 3.2 | Personnel training..... | 7 |
| 4 | Transport and storage | 7 |
| 4.1 | Testing upon acceptance | 7 |
| 4.2 | Packaging / return transport | 7 |
| 5 | Unpacking, Setup and Commissioning | 8 |
| 5.1 | Installation Site, Location of Use | 8 |
| 5.2 | Unpacking..... | 8 |
| 5.2.1 | Placing..... | 9 |
| 5.2.2 | Scope of delivery | 9 |
| 5.3 | Mains connection (optional)..... | 9 |
| 5.4 | Battery operation | 9 |
| 5.5 | Initial Commissioning..... | 10 |
| 5.6 | Adjustment..... | 10 |
| 5.7 | Adjustment..... | 10 |
| 6 | Operating elements | 13 |
| 6.1 | Keyboard overview | 13 |
| 6.1.1 | Models FOB-NS: | 13 |
| 6.1.2 | Models FOB-NL: | 14 |
| 6.2 | Overview of display | 15 |
| 6.2.1 | Models FOB-NS: | 15 |
| 6.2.2 | Models FOB-NL: | 15 |
| 7 | Operation | 16 |
| 7.1 | Simple weighing | 16 |
| 7.2 | Taring..... | 17 |
| 7.3 | Weighing units switch-over..... | 17 |
| 7.4 | Hold function (only "L" models) | 18 |
| 7.5 | Backlight of the display (only "L" models) | 19 |
| 8 | The menu | 20 |
| 8.1 | Call up menu | 20 |
| 8.2 | Navigation in the menu..... | 20 |
| 8.3 | Menu overview | 21 |
| 8.3.1 | Models FOB-NS: | 21 |
| 8.3.2 | Models FOB-NL: | 21 |
| 8.4 | Menu settings | 22 |
| 8.4.1 | Setting weighing units..... | 22 |
| 8.4.2 | Automatic switch-off function „AUTO OFF“ in stand-by mode | 24 |

| | | |
|-----------|---|-----------|
| 9 | Error messages | 26 |
| 10 | Servicing, maintenance, disposal | 26 |
| 10.1 | Cleaning..... | 26 |
| 10.2 | Servicing, maintenance | 26 |
| 10.3 | Disposal | 26 |
| 11 | Instant help | 27 |
| 12 | Declaration of Conformity | 28 |

1 Technical data

Models „FOB-NS“:

| KERN | FOB 0.5K-4NS | FOB 5K-3NS |
|--|-------------------------------|-------------|
| Readability (d) | 0.1 g | 1 g |
| Weighing range (max) | 500 g | 5000 g |
| Reproducibility | 0.1g | 1 g |
| Linearity | ± 0.2 g | ± 2 g |
| Weighing Units | g, lb, oz, ozt, dwt | |
| Recommended adjustment weight, not added (class) | 500 g (M1) | 5000 g (M1) |
| Warm-up time | 10 min | |
| Stabilization time (typical) | 2 sec. | |
| Operating temperature | + 10° C + 35° C | |
| Humidity of air | 25% - 95% (non-condensing) | |
| Housing (B x D x H) mm | 170 x 150 x 40 | |
| Weighing plate, stainless steel (mm) | 120 x 150 x 10 | |
| Weight kg (net) | 650 g | |
| Auto off | Options: 2, 3, 4, 5, min; off | |
| Battery | 9 V block | |
| Secondary voltage powerpack | 9 V / 100 mA | |
| IP protection | IP65 | |

Models „FOB-NL“:

| KERN | FOB 7K-4NL | FOB 10K-3NL | FOB 30K-3NL |
|--|----------------------------|--------------|---------------|
| Readability (d) | 0.5 g / 1 g | 1 g / 2 g | 2 g / 5 g |
| Weighing range (max) | 5 kg / 7.5 kg | 8 kg / 15 kg | 16 kg / 30 kg |
| Reproducibility | 0.5 g / 1 g | 1 g / 2 g | 2 g / 5 g |
| Linearity | ± 1.5 g / 3 g | ± 3 g / 6 g | ± 6 g / 15 g |
| Weighing Units | g, lb, oz, ozt, dwt | | |
| Recommended adjustment weight, not added (class) | 5 kg (M1) | 10 kg (M1) | 30 kg (M1) |
| Warm-up time | 30 min | 30 min | 30 min |
| Stabilization time (typical) | 2 sec. | | |
| Operating temperature | + 5° C + 35° C | | |
| Humidity of air | 25% - 95% (non-condensing) | | |
| Housing (B x D x H) mm | 285 x 255 x 90 | | |
| Weighing plate, stainless steel (mm) | 252 x 200 x 14 | | |
| Weight kg (net) | 3611 g | | |
| Auto off | 2 min | | |
| Battery | 4 x 1,5 V AA | | |
| Secondary voltage powerpack | 9 V / 100 mA | | |
| IP protection | IP67 | | |

2 Basic Information (General)

2.1 Proper use

The balance you purchased is intended to determine the weighing value of material to be weighed. It is intended to be used as a “non-automatic balance”, i.e. the material to be weighed is manually and carefully placed in the centre of the weighing plate. As soon as a stable weighing value is reached the weighing value can be read.

2.2 Improper Use

Do not use balance for dynamic weighing. In the event that small quantities are removed or added to the material to be weighed, incorrect weighing results can be displayed due to the “stability compensation“. (Example: Slowly draining fluids from a container on the balance.)

Do not leave permanent load on the weighing plate. This may damage the measuring system.

Impacts and overloading exceeding the stated maximum load (max) of the balance, minus a possibly existing tare load, must be strictly avoided. Balance may be damaged by this.

Never operate balance in explosive environment. The serial version is not explosion protected.

The structure of the balance may not be modified. This may lead to incorrect weighing results, safety-related faults and destruction of the balance.

The balance may only be used according to the described conditions. Other areas of use must be released by KERN in writing.

2.3 Warranty

Warranty claims shall be voided in case

- Our conditions in the operation manual are ignored
- The appliance is used outside the described uses
- The appliance is modified or opened
- mechanical damage and damage caused by media, liquids, natural wear and tear
- The appliance is improperly set up or incorrectly electrically connected
- The measuring system is overloaded

2.4 Monitoring of Test Resources

In the framework of quality assurance the measuring-related properties of the balance and, if applicable, the testing weight, must be checked regularly. The responsible user must define a suitable interval as well as type and scope of this test. Information is available on KERN's home page (www.kern-sohn.com) with regard to the monitoring of balance test substances and the test weights required for this. In KERN's accredited DKD calibration laboratory test weights and balances may be calibrated (return to the national standard) fast and at moderate cost.

3 Basic Safety Precautions

3.1 Pay attention to the instructions in the Operation Manual



Carefully read this operation manual before setup and commissioning, even if you are already familiar with KERN balances.

All language versions contain a non-binding translation.

The original German is binding.

3.2 Personnel training

The appliance may only be operated and maintained by trained personnel.

4 Transport and storage

4.1 Testing upon acceptance

When receiving the appliance, please check packaging immediately, and the appliance itself when unpacking for possible visible damage.

4.2 Packaging / return transport



- ⇒ Keep all parts of the original packaging for a possibly required return.
- ⇒ Only use original packaging for returning.
- ⇒ Prior to dispatch disconnect all cables and remove loose/mobile parts.
- ⇒ Reattach possibly supplied transport securing devices.
- ⇒ Secure all parts such as the glass wind screen, the weighing plate, power unit etc. against shifting and damage.

5 Unpacking, Setup and Commissioning

5.1 Installation Site, Location of Use

The balances are designed in a way that reliable weighing results are achieved in common conditions of use.

You will work accurately and fast, if you select the right location for your balance.

Therefore, observe the following for the installation site:

- Place the balance on a firm, level surface;
- Avoid extreme heat as well as temperature fluctuation caused by installing next to a radiator or in the direct sunlight;
- Protect the balance against direct draughts due to open windows and doors;
- Avoid jarring during weighing;
- Protect the balance against high humidity, vapours and dust;
- Do not expose the device to extreme dampness for longer periods of time. Non-permitted condensation (condensation of air humidity on the appliance) may occur if a cold appliance is taken to a considerably warmer environment. In this case, acclimatize the disconnected appliance for ca. 2 hours at room temperature.
- Avoid static charge of goods to be weighed or weighing container.

Major display deviations (incorrect weighing results) may be experienced should electromagnetic fields (e.g. due to mobile phones or radio equipment), static electricity accumulations or instable power supply occur. Change location or remove source of interference.

5.2 Unpacking

Carefully remove the weighing balance from the packaging and install it at the designated work place.

5.2.1 Placing

The balance must be installed in a way that the weighing plate is exactly in horizontal position.

5.2.2 Scope of delivery

Serial accessories:

- Balance
- Weighing plate
- Mains adapter (optional)
- Protective cover
- Operating manual

5.3 Mains connection (optional)

The balance may be operated via the optional mains adapter. The stated voltage value must be the same as the local voltage.

Only use original KERN mains adapters. Using other makes requires consent by KERN.


5.4 Battery operation

Unscrew battery cover on the bottom of the housing (see figure 1).


- 9 V block battery (FOB-NS) or
- 4 x 1.5V AA batteries (FOB-NL)

Put battery cover back in place and tighten it.

Fig. 1:

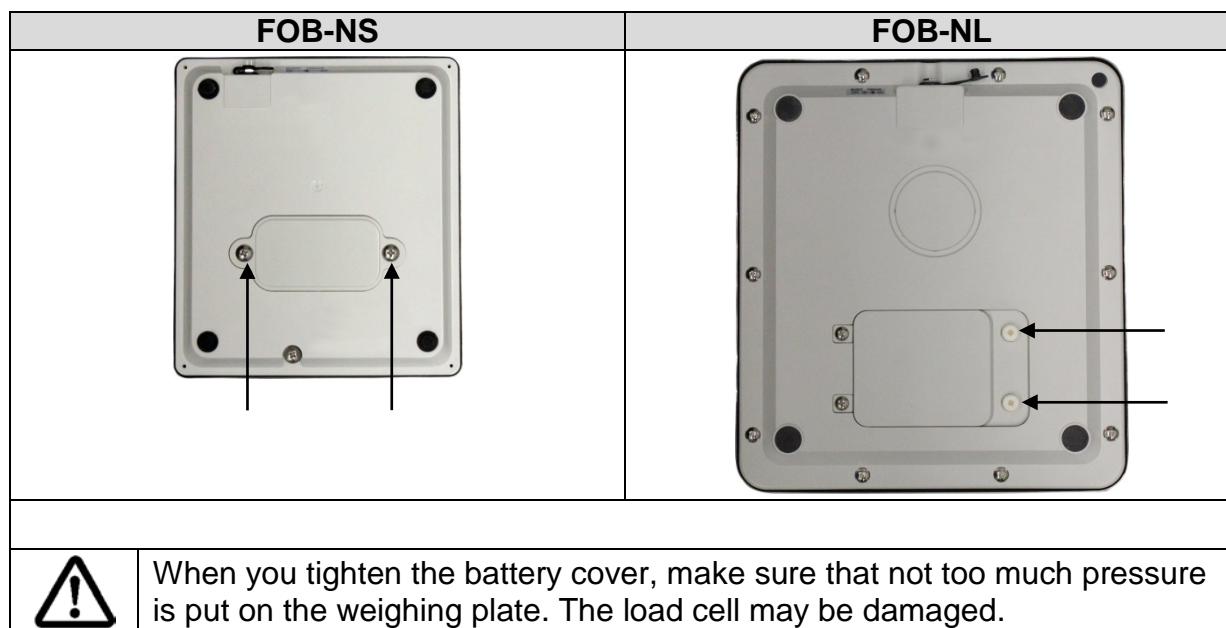

In the menu you can activate the AUTO-OFF function (see chap. 8.4.2 "Automatic switch-off function"). According to the selected settings, the balance switches automatically off in order to spare the battery.

The empty battery is indicated on the display by „**LobAt**“. Press button  and change the battery/batteries immediately.

If the balance is not used for a longer time, take out the battery/ies and store it/them separately. Leaking battery liquid could damage the balance.

5.5 Initial Commissioning

In order to obtain exact results with the electronic balances, your balance must have reached the operating temperature (see warming up time chap. 1). During this warming up time the balance must be connected to the power supply (mains or battery).

The accuracy of the balance depends on the local acceleration of gravity.

Strictly observe hints in chapter Adjustment.

5.6 Adjustment

As the acceleration value due to gravity is not the same at every location on earth, each balance must be coordinated - in compliance with the underlying physical weighing principle - to the existing acceleration due to gravity at its place of location (only if the balance has not already been adjusted to the location in the factory). This adjustment process must be carried out for the first commissioning, after each change of location as well as in case of fluctuating environment temperature. To receive accurate measuring values it is also recommended to adjust the balance periodically in weighing operation.

5.7 Adjustment

The adjustment should be made with the recommended adjustment weights (see chap. 1 "Technical data").












Procedure when adjusting:

Observe stable environmental conditions.












A warming up time (see chapter 1; Technical Data) is required for stabilization.

Ensure that there are no objects on the weighing plate.

Models FOB-NS:

| Balance display | Operation |
|--|---|
|  ↓  (example) | <ul style="list-style-type: none">⇒ Switch off the balance⇒ Press and hold , press  3x at the same time, release  - an internal value is displayed. |
|   ↓  (example) | <ul style="list-style-type: none">⇒ Press , "0" is displayed⇒ Put adjustment weight in the centre of the weighing plate and press , "CAL" is displayed, followed by the value of the adjustment weight.⇒ Take away adjustment weight⇒ The balance changes into weighing mode.⇒ Adjustment has now been completed successfully. |
|  | |


Models FOB-NL:




| Balance display | Operation |
|--|---|
|  <p style="text-align: center;">↓</p>  <p style="text-align: center;">(example)</p> | <ul style="list-style-type: none"> ⇒ Switch off the balance ⇒ Press and hold , press  3x at the same time, release  - an internal value is displayed. |
|   <p style="text-align: center;">↓</p>  <p style="text-align: center;">(example)</p>  | <ul style="list-style-type: none"> ⇒ Press , "0" is displayed ⇒ Put adjustment weight in the centre of the weighing plate, wait for stability display and press , ⇒ "CAL" is displayed, followed by the value of the adjustment weight. ⇒ Take away adjustment weight ⇒ The balance changes into weighing mode. ⇒ Adjustment has now been completed successfully. |

6 Operating elements

6.1 Keyboard overview

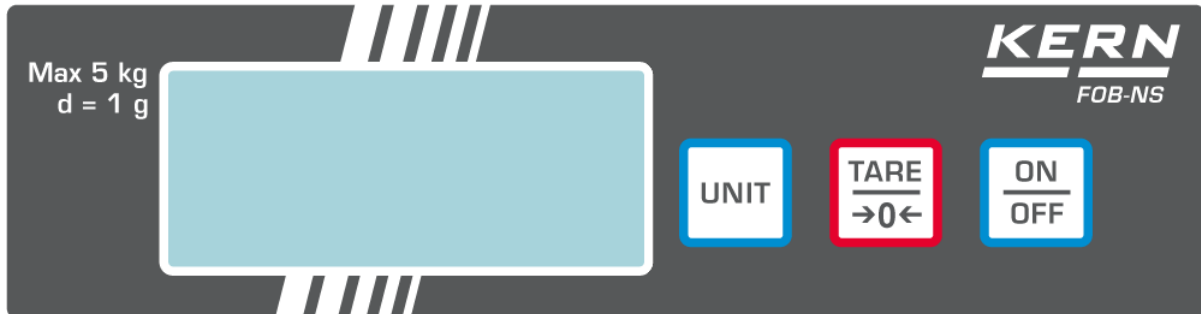



6.1.1 Models FOB-NS:



| Button | Designation | Pressed once and released | |
|---|-------------|---|---|
|  | [ON/OFF] | <ul style="list-style-type: none"> • Turn on/off • Call up adjustment (press and hold button) | |
|  | [TARE] | <ul style="list-style-type: none"> • Taring | In menu: <ul style="list-style-type: none"> • Passing through menu items from top to bottom |
|  | [UNIT] | <ul style="list-style-type: none"> • Weighing units switching over • Invoke adjustment | <ul style="list-style-type: none"> • Passing through menu items from left to right |

6.1.2 Models FOB-NL:



| Button | Designation | Pressed once and released | |
|---|-------------|--|---|
|  | [ON/OFF] | <ul style="list-style-type: none"> • Turn on/off • Call up adjustment (press and hold button) | |
|  | [TARE] | <ul style="list-style-type: none"> • Taring • Display backlight (press button long time) | In menu: <ul style="list-style-type: none"> • Passing through menu items from top to bottom |
|  | [UNIT] | <ul style="list-style-type: none"> • Weighing units switching over • Call up adjustment (press shortly 3x) | <ul style="list-style-type: none"> • Passing through menu items from left to right |
|  | [HOLD] | <ul style="list-style-type: none"> • Call up hold function | |


6.2 Overview of display

6.2.1 Models FOB-NS:



| Display | Description |
|---------------------|------------------------|
| g, lb, oz, ozt, dwt | Display weighing units |
| ○ | Stability display |



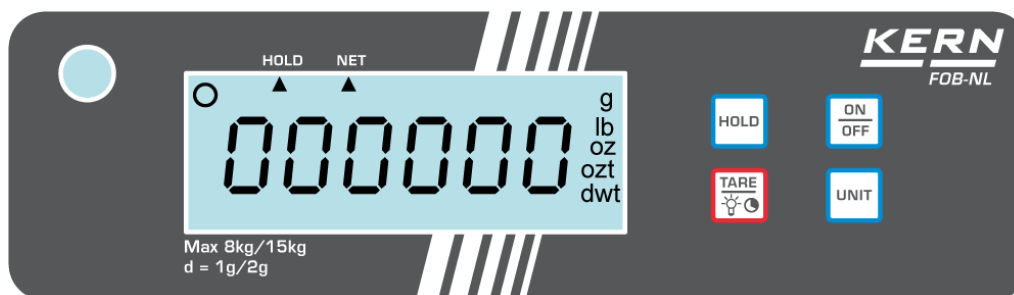




6.2.2 Models FOB-NL:



| Display | Description |
|---------------------|------------------------|
| g, lb, oz, ozt, dwt | Display weighing units |
| ○ | Stability display |
| HOLD | Display hold function |
| NET | Display net weight |







7 Operation

7.1 Simple weighing

| Balance display | Operation |
|---|---|
|  | <p>⇒ Start balance by pressing .</p> <p>The balance will carry out a self-test.</p> <p>Wait for „0“ display</p> |
|  | <p>⇒ If the balance should not exactly display "0" despite the relieved weighing pan, press</p> <p> ("L" models) or</p> <p> ("S" models).</p> <p>The balance returns to „0“</p> |
|  <p>(example)</p> | <p>⇒ Place goods to be weighed on balance.</p> <p>Wait until the stability display appears.</p> <p>Read weighing result.</p> |
| | <p>⇒ To switch off the balance press shortly .</p> |

7.2 Taring

The dead weight of any weighing container may be tared away by pressing a button, so that the following weighing procedures show the net weight of the goods to be weighed.

| Balance display | Operation |
|--|---|
|  <p>(example)</p> | <p>⇒ Deposit weighing vessel. The weight of the container is displayed.</p> |
|  | <p>⇒ Press  ("L" models) or  ("S" models), the zero display appears. The weight of the container is now internally saved.</p> |
|  <p>(example FOB-NS)</p>  <p>(example FOB-NL)</p> | <p>⇒ Place goods to be weighed in the weighing container. The net weight of the goods to be weighed is displayed.</p> <p>For L models, a triangle appears below the NET symbol.</p> |

7.3 Weighing units switch-over








According to the requirements the balance can be switched over into different units. These are set in the menu.

In weighing mode, use  to change between the set units.








7.4 Hold function (only "L" models)

The balance has an integrated standstill function (mean value calculation). With this it is possible to weigh unstable samples to be weighed exactly. There are 2 possibilities:

1.

| Balance display | Operation |
|--|--|
|  | <ul style="list-style-type: none"> ⇒ Start balance by pressing . The balance will carry out a self-test. ⇒ Wait for „0“ display |
|   (example) | <ul style="list-style-type: none"> ⇒ Put sample to be weighed in place and press ; "HOLD" will appear and a small triangle flashes. During this time, an average value is recorded. ⇒ The triangle will stop flashing, the stability display appears and the weight value obtained is displayed. |
|  | <ul style="list-style-type: none"> ⇒ By pressing  the balance returns to weighing mode. The triangle disappears. |

2.

| Balance display | Operation |
|---|--|
|  | <p>⇒ Start balance by pressing .</p> <p>The balance will carry out a self-test.</p> <p>⇒ Wait for „0“ display</p> |
|   <p>(example)</p> | <p>⇒ Press , "HOLD" will appear and a small triangle flashes. During this time put samples to be weighed in place.</p> <p>⇒ The stability display will appear after a short time, the triangle will stop flashing and the obtained weight value is displayed.</p> |
|  | <p>⇒ By pressing  the balance returns to weighing mode. The triangle disappears.</p> |

7.5 Backlight of the display (only "L" models)



The balance has the ability to turn the backlight of the display on or off.

For this purpose press  for approx. 3 sec.

8 The menu

8.1 Call up menu




„L“-Models:

- Switch off the balance
- Press and hold  and press  3x at the same time, then release both buttons.

„S“-Models:


The menu is accessed by pressing  in weighing mode for approx. 3 seconds.

8.2 Navigation in the menu

| Button | Direction in the menu | Description |
|---|-----------------------|--|
|  („L“-models)  („S“-models) | ↓ | <ul style="list-style-type: none"> • Passing through menu items from top to bottom • Confirm selection |
|  | → | <ul style="list-style-type: none"> • Passing through menu items from left to right |


8.3 Menu overview

8.3.1 Models FOB-NS:

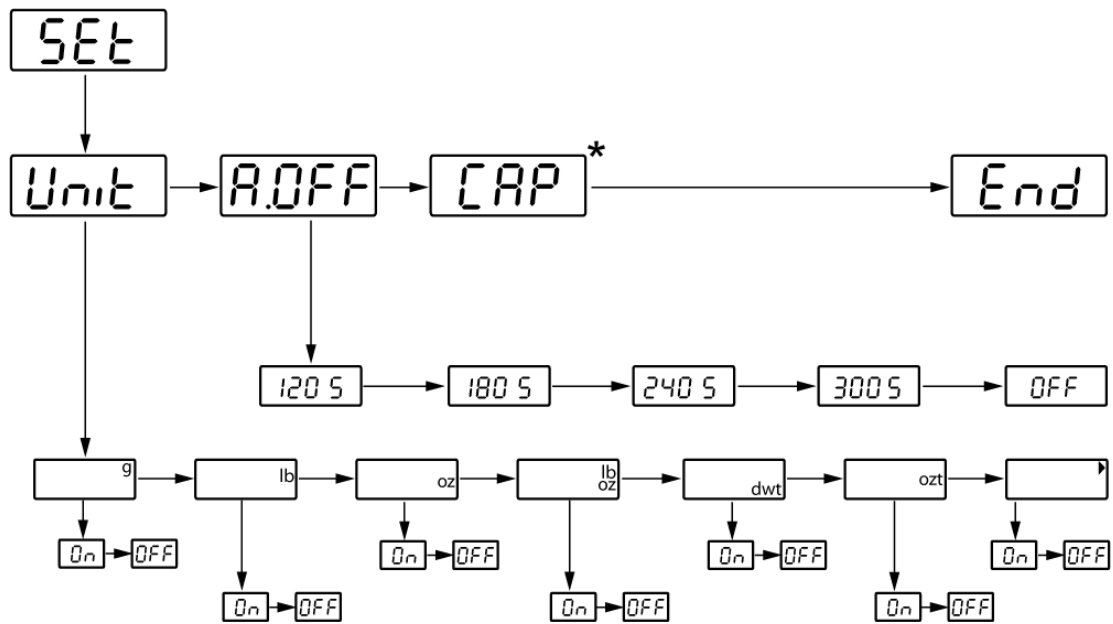






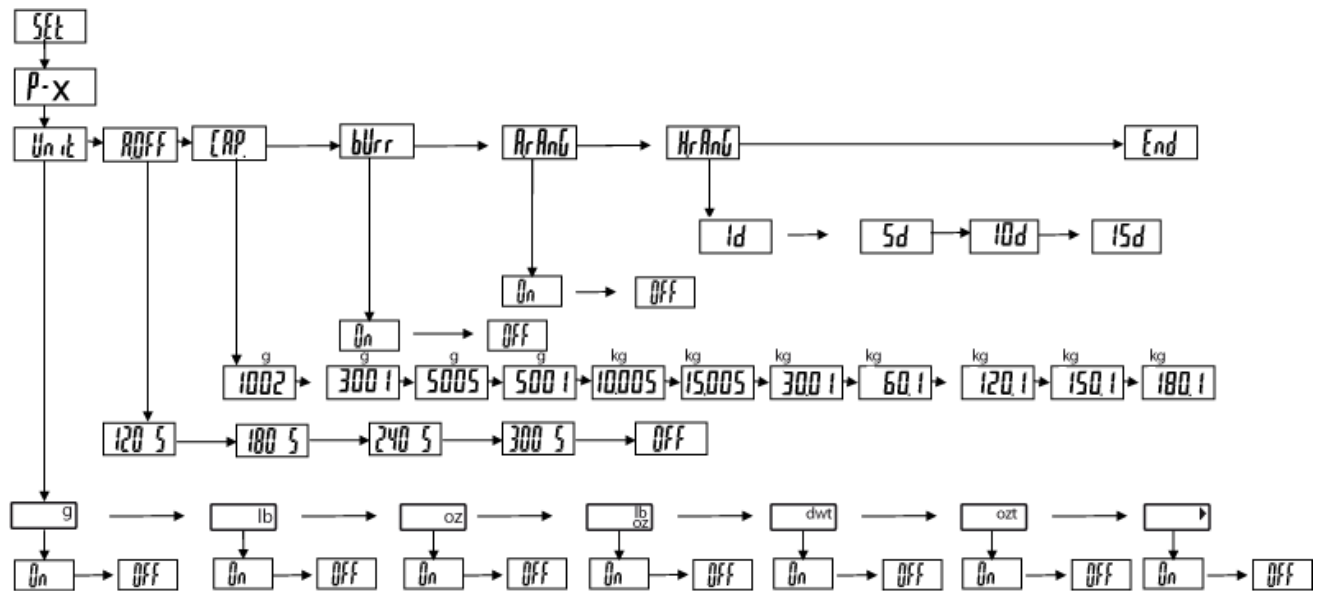











* not documented













8.3.2 Models FOB-NL:




8.4 Menu settings

8.4.1 Setting weighing units







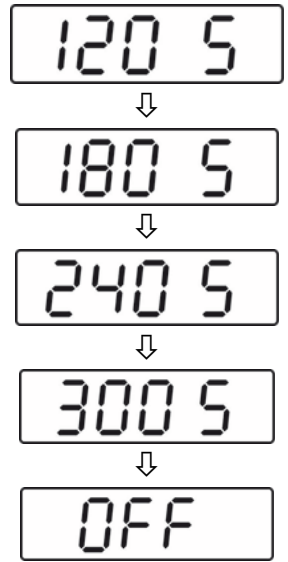



| Balance display | Operation |
|---|--|
|  | <p>FOB-S:</p> <p>⇒ In weighing mode press  button for approx. 3 seconds. „SEt“, followed by „Unit“ is displayed</p> <p>FOB-L:</p> <p>⇒ Switch off the balance</p> <p>Press and hold  and press  3x at the same time, then release both buttons.</p> |
|  | <p>⇒ Press  or  again, the weighing unit „g“ is displayed</p> |
|  | <p>⇒ Use  to change to the desired unit</p> |
|  | <p>⇒ Press  or , "OFF" is displayed</p> |
|  | <p>⇒ Use  to change to „On“</p> |
|  | <p>⇒ Press  or , the selected unit is displayed and set.</p> |











| | |
|---|---|
|  | ⇒ Press  repeatedly until „Unit“ is displayed |
|  | ⇒ Press  , „A.Off“ will be shown |
|  | ⇒ Press  , „CAP.“ is displayed |
|  | ⇒ Press  , „End“ is displayed |
|  | ⇒ Press  or  to return to weighing mode |
| | ⇒ Use  to change between the set units |


| | |
|--|--|
|  | In order to switch off the units display, proceed as described above and set the selected unit to „Off“. |
|--|--|

8.4.2 Automatic switch-off function „AUTO OFF“ in stand-by mode







The balance offers the possibility of the automatic switch-off, when the balance is in stand-by mode. The switch-off time may be selected as follows:

| Balance display | Operation |
|---|---|
|  | <p>FOB-S:</p> <p>⇒ In weighing mode press  button for approx. 3 seconds. „SEt“, followed by „Unit“ is displayed</p> <p>FOB-L:</p> <ul style="list-style-type: none"> • Switch off the balance • Press and hold  and press  3x at the same time, then release both buttons. |
|  | <p>⇒ Press  „AOFF“ is displayed</p> |
|  | <p>⇒ Press  or , the current setting will be displayed.</p> <p>⇒ Select the desired setting by pressing :</p> <p>120s = Auto off after 120 seconds 180s = Auto off after 180 seconds 240s = Auto off after 240 seconds 300s = Auto off after 300 seconds OFF = Auto off switched off</p> |

| | |
|---|--|
|  | ⇒ Use  or  to adopt selection, „AOFF“ is displayed |
|  | ⇒ Press  „CAP“ is displayed |
|  | ⇒ Press  again, „End“ is displayed |
|  | ⇒ Using  or  the balance returns to weighing mode. The setting is saved. |

| | |
|---|--|
|  | The auto-off function is only possible in battery operation. In mains operation this function is turned off. |
|---|--|

9 Error messages

| | | |
|---|---------------------------|--|
|  | Battery empty | Insert new battery or connect the balance to power supply |
|  | Weighing range exceeded | Remove load and set balance to zero with  or  , if necessary |
|  | Zeroing range not reached | Increase the load, if the error message remains, please contact your retailer |
|  | Software error | Contact your retailer |

10 Servicing, maintenance, disposal

10.1 Cleaning

Before cleaning, please disconnect the appliance from the operating voltage.

- ⇒ Clean the stainless-steel parts with a soft cloth soaked with a cleaning agent suitable for stainless steel.
- ⇒ For stainless steel parts do not use any cleaning agents which contain sodium hydroxide solution, acetic, hydrochloric, sulphuric or citric acid.
- ⇒ Do not use metal brushes or cleaning sponges of steel wool, as this causes superficial corrosion.

Spilled weighing goods must be removed immediately.

10.2 Servicing, maintenance

The appliance may only be opened by trained service technicians who are authorized by KERN.

Before opening, disconnect from power supply.

10.3 Disposal

Disposal of packaging and appliance must be carried out by operator according to valid national or regional law of the location where the appliance is used.

11 Instant help

In case of an error in the program process, briefly turn off the balance and disconnect from power supply. The weighing process must then be restarted from the beginning.

Help:

Fault

Possible cause

The displayed weight does not glow.

- The balance is not switched on.
- The mains supply connection has been interrupted (mains cable not plugged in/faulty).
- Power supply interrupted.
- (Rechargeable) batteries are inserted incorrectly or empty
- No (rechargeable) batteries inserted.

The displayed weight is permanently changing

- Draught/air movement
- Table/floor vibrations
- Weighing plate has contact with other objects.
- Electromagnetic fields / static charging (choose different location/switch off interfering device if possible)

The weighing result is obviously incorrect

- The display of the balance is not at zero
- Adjustment is no longer correct.
- Great fluctuations in temperature.
- Warm-up time was ignored.
- Electromagnetic fields / static charging (choose different location/switch off interfering device if possible)

Should other error messages occur, switch balance off and then on again. If the error message remains inform manufacturer.

12 Declaration of Conformity

To view the current EC/EU Declaration of Conformity go to:

www.kern-sohn.com/ce